



Technical data sheet TDS0068

PREMIER HIGH RESOLUTION METHANE SENSOR CERTIFIED VERSIONS TYPES MSH-P-HR and MSHia-P-HR

Great Britain
Europe
France
Germany
Italy
Switzerland
USA

Patent Numbers
GB 2 401 432 & GB 2 403 291
EP 1544603 & EP 1818667-Pending
EP [FR] 1544603
EP [DE] 1544603
EP [I] 11544603
EP [CH] 1544603
7, 244, 939
Other World Patents Pending



"Platinum Series"

FEATURES

- ★ High resolution infrared sensor measures methane from 0 to 100% volume with resolution of 0.01 % for 0-10% methane and 0.1% for 10-100% volume.
- ★ Combines all the features of the well-proven range of Premier hydrocarbon sensors, enabling the accurate measurement of 0-100% vol. methane with one sensor.
- ★ Contains all the necessary optics, electronics and firmware to provide a linearised, temperature-compensated output.
- ★ Choice of output format – digital output, direct pellistor replacement or industry standard 0.4 to 2 volts.
- ★ Sensors can be factory configured to customer specification.
- ★ All sensor types are user configurable using configuration equipment available from Dynamant.
- ★ Fast track route for original equipment manufacturers to introduce the latest infrared technology – without any specialist knowledge.
- ★ Internal Flash memory allowing sensor firmware updates via configuration equipment.

Replaces:

a) An infrared 0-5% vol. methane sensor and a 0-100% vol. methane sensor.

or

b) A set of catalytic beads for LEL methane and a set of catalytic beads for % vol. methane.



Dynamant Limited

Premier House · The Village · South Normanton · Derbyshire · DE55 2DS · UK.

Tel: 44 (0)1773 864580 · Fax: 44 (0)1773 864599

email: sales@dynamant.com · www.dynamant.com

CERTIFICATION DETAILS

European ATEX Certification	Sensor type MSH-P	Sensor type MSHia-P
Approval body	SIRA	
Certificate Number	SIRA 04ATEX1357U	
Test Standards	EN60079-0:2006, EN60079-1:2004, EN60079-11:2007, EN60079-26:2006	
Certification Codes	I M2 Ex d I & II 2 G Ex d IIC	I M1 Ex d+ia I Ma & II 2 G Ex d IIC Gb
Input parameters	0.8W max, 30V max.	Ui=6V dc, Pi=0.8W
Operating temperature	-20°C to +60°C	
International IECEx Certification	Sensor type MSH-P	Sensor type MSHia-P
Approval body	SIRA	
Certificate Number	IECEx SIR 05.0053U	
Test Standards	IEC 60079-0:2004, IEC60079-1:2003, EN60079-26:2006	
Certification Codes	Ex d I & Ex d IIC	Ma Ex d+ia I & Gb Ex d IIC
Input parameters	0.8W max, 30V max.	Ui=6V dc, Pi=0.8W
Operating temperature	-20°C to +60°C	
North American Certification	Sensor type MSH-P	
Approval body	Underwriters Laboratory Inc.	
File Reference	E229543	
Test Standards	UL913 Fifth Edition	
Hazardous Locations	Class 1 Groups A, B, C and D, T4 with 60°C ambient	
Input parameters are defined for certification purposes only, refer to the "Specification" table on page 9 for the sensor operating voltage and temperature range.		

DESCRIPTION

Dynamant infrared sensors operate by using the NDIR principle to monitor the presence of the target gas. The sensor contains a long life tungsten filament infrared light source, an optical cavity into which gas diffuses, a dual temperature compensated pyroelectric infrared detector, an integral semiconductor temperature sensor and electronics to process the signals from the pyroelectric detector .

Two versions are available:-

3 Pin Version - Pellistor Replacement Infrared

These sensors provide a pellistor style linearised, temperature-compensated output as shown in Graph 1.


They can either be supplied pre-set to customer specification or may be configured by the user by means of a configuration unit available from Dynamant Ltd. The output signal can be set to rise or fall with increase in the gas level.

5 Pin Version - Multi-Purpose Range

This version of the sensor provides maximum user flexibility by providing the following output options:-

- ★ Industry Standard 0.4 to 2 volt linearised, temperature-compensated output as shown in Graph 2, or alternative voltages for zero and full-scale outputs.
- ★ Digital output for direct communications with instrument electronics.
- ★ Rising or falling output with increasing gas level for the pellistor replacement, bridge output as shown in graph 1.

The digital output is a UART format comprising 8 data bits, 1 stop bit and no parity. Refer to specification for available baud rates.

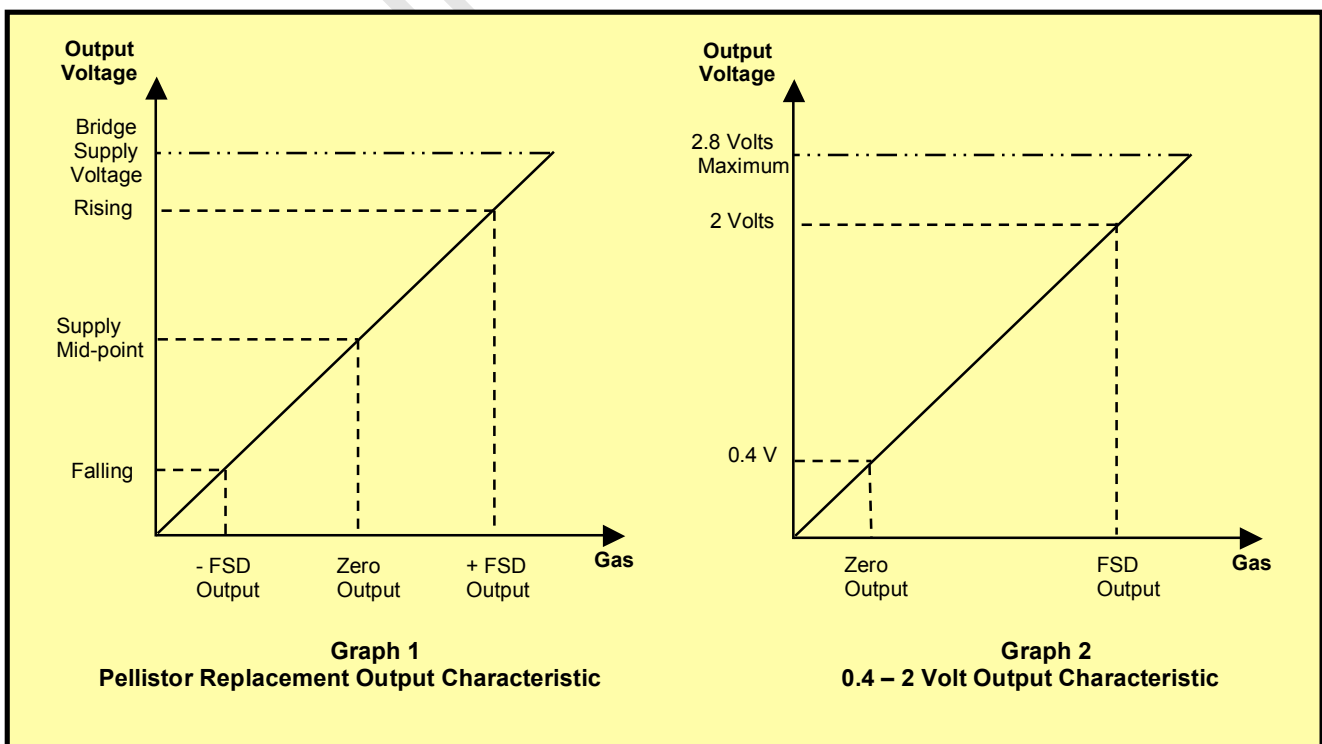


Relative Response Characteristics

The Premier High Resolution methane sensor is calibrated to provide an output signal linearised for 0-100% volume methane during manufacture.

However, the sensor will also respond to a range of other hydrocarbon gases. The following graph shows the relative response to some of the common hydrocarbons.

These characteristics can be used as a guide to setting up the associated instrument alarm levels.

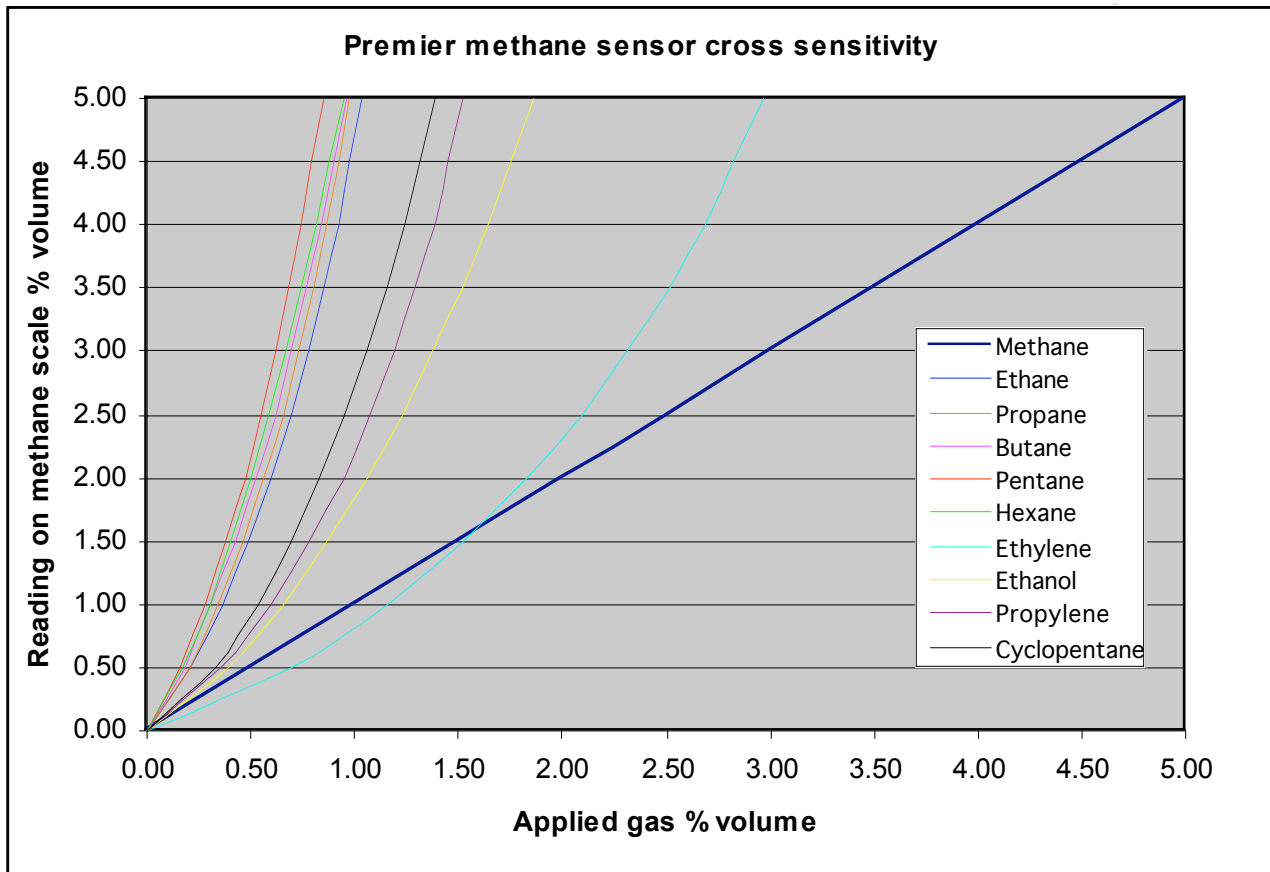


Note – Refer to data sheet TDS0050 for additional cross reference data


Temperature Compensation

The Premier sensor is temperature compensated over the range of -20°C to +50°C.

The output variation is $\pm 0.1\%$ volume methane or $\pm 10\%$ of the reading for the range 0 to 10% volume, whichever is greater.

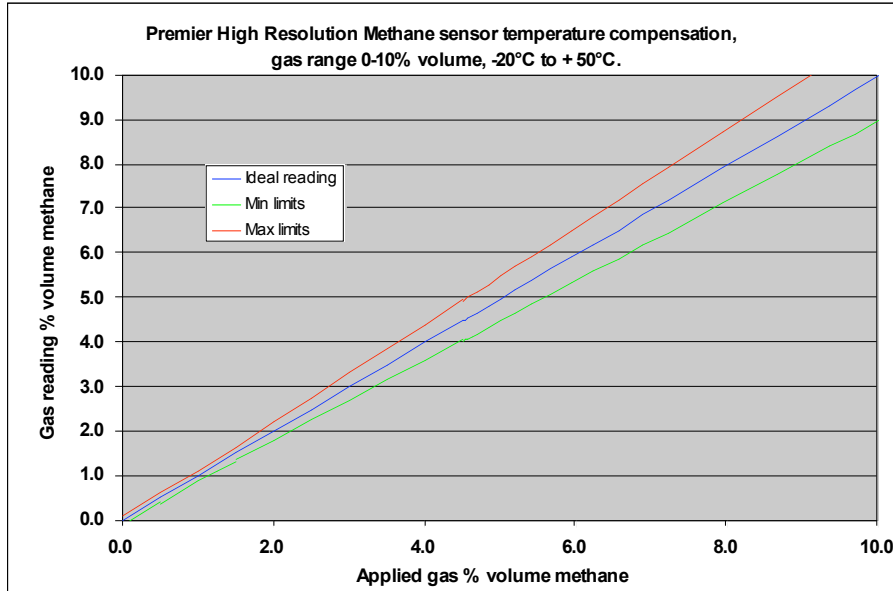



For the range 10% to 100% volume the output variation is $\pm 10\%$ of the reading.

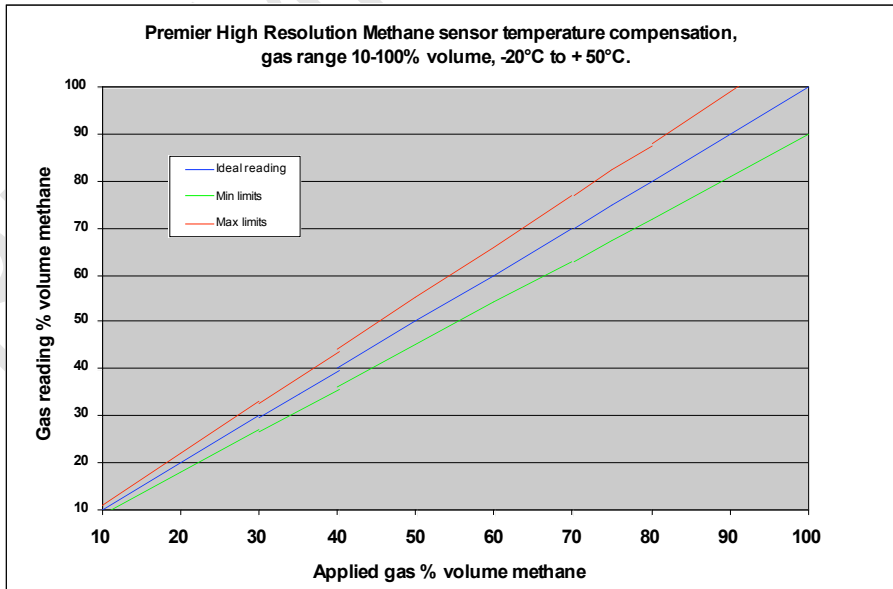

Linearity

The linearity at ambient temperature is $\pm 10\%$ of the reading across the full measuring range.

The following graphs show actual test data for linearity over the ranges 0-10% volume and 10-100% volume.

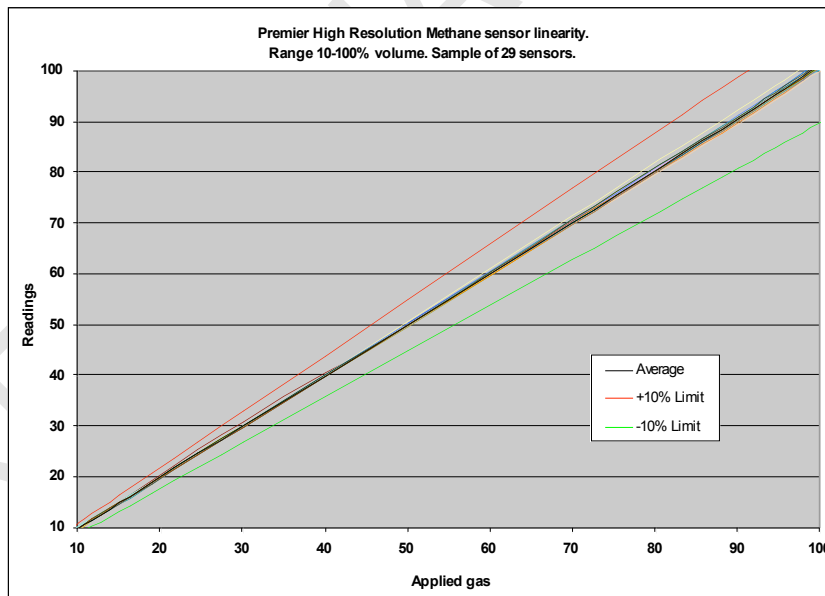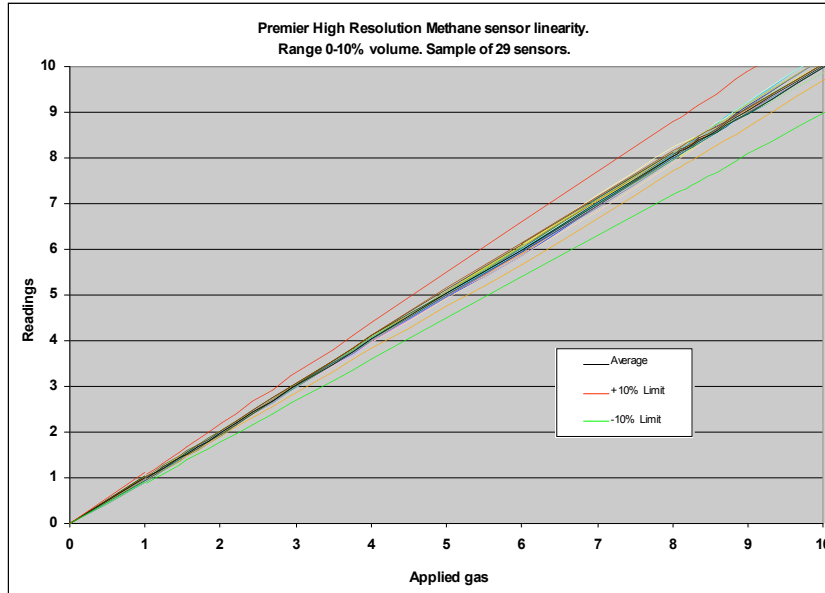

Calibration options

Dynamant recommend a maximum interval of 12 months between calibration checks. A small amount of zero drift can be accommodated by re-zeroing the gas detector against the sensor. The degree of drift that is acceptable should be determined by the user. Note that the subsequent change in gas reading will be greater than the change in zero reading. If the sensor requires either a "Zero" or "Span" adjustment, there are three methods that can be used:

- 1) By using the "Premier Configuration Unit"
When used in conjunction with dedicated PC software, this device uses the data communication pins on the sensor to provide a means of calibration. Refer to data sheet TDS0043 for additional information.
- 2) By using the data communications pins and software written in accordance with the protocol supplied by Dynamant.
- 3) By using the "Manual Calibration" feature available with firmware version 1.5.2R.
"Zero" and "Span" operations can be performed by momentarily connecting the data communication pins to the negative supply pin. Refer to data sheet TDS0064 for full instructions. The "Manual Calibration" option must be specified when the sensors are ordered.

Sensor warm-up time

When power is first applied to the sensor, the voltage at the output pin is held at a pre-determined level. The default setting for this start-up value is the "zero gas" value. This condition is maintained for a default "warm-up" time of 15 seconds, after this time the output voltage represents the calculated gas value. Sensors can take up to 1 minute to indicate the correct gas reading.

Note: the sensor can output any reading from -100% full-scale to +200% full-scale in the first minute.

The output value that is read using the communications pins is always held at zero during the "warm-up" time.

Both the voltage at the output pin during the "warm-up" time, and the duration of the "warm-up" time can be pre-programmed to alternative values at the time of ordering sensors.

Temperature transients and gas flow rates.

The Premier sensor employs a pyroelectric detector, the output from which can be disrupted by sudden changes in temperature. If there is an excessive change in the ambient temperature, gas sample temperature or flow rate, then the output signal will be momentarily frozen. Correct operation is restored when the effects of the transient have settled. Rates of change in the ambient temperature should be restricted to 2°C/minute and gas flow rates kept below 600 cc/minute.

Power supply considerations

The sensor power supply rise time must be less than 50 mS to ensure correct operation. Operation outside the range of 3 – 5 V dc will result in either fault indication, or the sensor will not function correctly.

Sensor over-range condition

The sensor will continue to provide an output up to a pre-determined percentage of the full scale value; at this point the reading is clamped, regardless of any further increase in detected gas level. The over-range value should be specified when ordering; choose from the following values 100%, 125%, 150% and 200%. The linearity of the output is only guaranteed up to the full scale for the sensor; the over-range condition for the host instrument should therefore be determined by the user.

Sensor fault indication

The sensor constantly performs checks on the internal memory contents, the incoming supply voltage and the analogue signal values. These checks are used to ensure that the sensor is operating within its correct parameters, and that no internal faults have developed.

If a fault condition is detected, the output value is set to -100% full-scale. In the case of a sensor with a voltage output that is scaled, 0.4 – 2.4V, for example, the output will be set to 0V under fault conditions.

It is not recommended to choose an output voltage of 0V for zero-gas, because the fault condition cannot then be distinguished from the zero-gas condition.

The output value that is read when using the communications pins, instead of the voltage output pin, will be set to -100% full-scale under fault conditions.

As mentioned in the “Sensor warm-up time” section above, the voltage at the output pin during the warm-up time can be specified when ordering sensors. It should be noted that if a start-up voltage is chosen that represents the zero-gas condition, then should a fault subsequently develop leaving the sensor unable to drive the output to -100% full-scale, this condition cannot be detected by the host instrument.

The start-up voltage that is equivalent to zero-gas was chosen as the default setting because, in a large number of applications, the host instrument would otherwise indicate fault during the warm-up period.

Warranty information

All Dynament Premier sensors carry a two year warranty against defects in materials and workmanship. The warranty is invalidated if the sensors are used under conditions other than those specified in this data sheet.

Particular attention should be paid to the following criteria:


- **Observe the correct supply polarity**
- **Do not exceed the maximum rated supply voltage of 5V**
- **Do not solder directly to the sensor pins**
- **Do not expose the sensor to corrosive gases**
- **Do not allow liquids to enter the sensor**

SPECIFICATION @ 20°C (68°F) ambient temperature

Operating Voltage Range:	3.0 – 5.0 V d.c.
Operating Current:	Constant current operation, current range 75 – 85mA
Programmable Output Voltage Ranges:	Voltage Output Types – 0v to 2.8 volts d.c. Bridge Output Types – 0v to Bridge Supply Voltage
Methane measuring range:	0 – 100% volume
Resolution:	0.01% volume for the range 0-10% volume methane and 0.1% volume for the range 10-100% volume. Output voltage resolution 42.7 μ V.
Linearity:	The output is linear within \pm 10% from 0-100% volume.
Warm up time:	To final zero \pm 2% full-scale: 1 minute
Response Time T₉₀:	<30s
Zero Repeatability:	\pm 0.05% volume methane
Span Repeatability:	\pm 0.1% volume methane at 5% applied gas. \pm 2% volume methane at 100% applied gas.
Long term zero drift:	\pm 0.05% volume methane per month
Operating temperature range:	-20°C to +50°C (-4°F to 122°F)
Temperature performance over the range -20°C to +50°C (-4°F to 122°F):	\pm 0.1% volume methane or \pm 10% of the reading for the range 0 to 100% volume, whichever is greater.
<small>Note: may not be applicable when using gas cross-reference factors</small>	
Storage temperature range:	-20°C to +50°C (-4°F to 122°F)
Humidity range:	0 to 95% RH non-condensing.
Digital signal format:	8 data bits, 1 stop bit, no parity. 2.8V logic level
Standard baud rates:	38,400, 19,200, 9600
User configurable parameters and functions:	Zero output voltage Full-scale output voltage Positive or negative going output Sensor 'zero' function Sensor 'span' function Over-range value
MTBF:	> 5 years
Weight :	15 grams

MECHANICAL DETAIL

NOTES

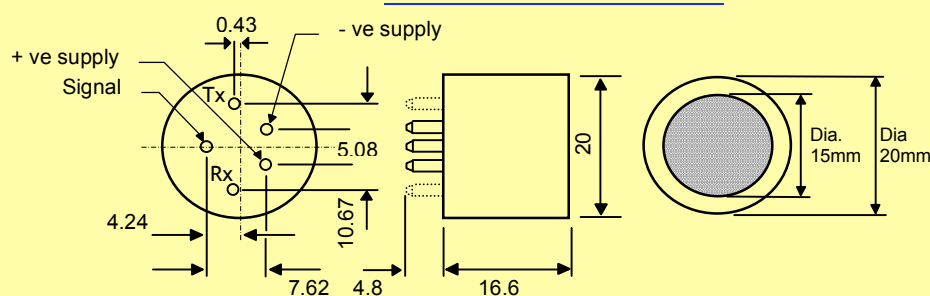

Pins viewed from underside
Diameter of pins = 1.5mm
Tx & Rx communication connections are available as either pads or pins

1. DIMENSIONS WITHOUT TOLERANCES ARE NOMINAL.
2. RECOMMENDED PCB SOCKET WEARNES CAMBION LTD CODE: 450-3326-01-06-00.
3. WEIGHT: 15g
4. USE ANTI-STATIC PRECAUTIONS WHEN HANDLING
5. DO NOT CUT PINS
6. DO NOT SOLDER DIRECTLY TO PINS

NOTE – The above pin configuration is shown for the POSITIVE version of the sensor. The NEGATIVE version has the +ve and –ve supply pin positions exchanged. See ordering details.

Dynamant reserve the right to alter technical specifications without prior notice.

Ordering Details

In order to completely specify the type of sensor that is required, the customer needs to provide the following information:-

- An Order Code (see below) that specifies the sensors' basic physical and electrical characteristics.
- The sensor configuration requirements.

Available sensor options:

F = Replaceable, self adhesive microporous PTFE filter

EXAMPLE OF ORDER CODES

MSH – P / HR / 3 / B / P / F

Option

FILTER : BLANK = OMITTED
 F = FITTED

SUPPLY POLARITY : P = Positive
 N = Negative

OUTPUT TYPE : B = Bridge
 V = Voltage

NUMBER OF PINS : 3 or 5

SENSOR TYPE : HR = High Resolution

PREMIER SENSOR

TYPE MSH or MSHia (For Mining M1 applications only)

CONFIGURATION OPTIONS

(To be stated on customer order in addition to the Order Code)

1. Output voltage for zero.
2. Output voltage for span.
3. Rising or falling output voltage with increasing gas level (for "Bridge" outputs)
4. Sensitivity e.g. 100 mV = 100 % volume CH₄ for "Bridge" outputs, 0.4 – 2.4V = 100% volume methane for "Voltage" output sensors.
5. Communication speed – 38,400 baud (default), specify alternative rate if required.
6. Over-range value: 100%, 125%, 150% and 200% of full-scale value.

Pellistor Replacement - Explanation of Positive & Negative Polarity

Typical Pellistor Pinout

Premier Negative Polarity Option

Use where the DET pin of the existing pellistor is connected to the Negative of the pellistor bridge supply.

Premier Positive Polarity Option

Use where DET pin of the existing pellistor is connected to the Positive of the pellistor bridge supply.

Note – On the 3 pin version of the sensor, the RX and TX connections are pads, not pins.

TDS 0068

Issue 1.0

16/4/09

Change Note:N/A

Page 10 of 10